



NITRATE NITROGEN TABLET KIT

OCTA-SLIDE 2, 0-15 ppm

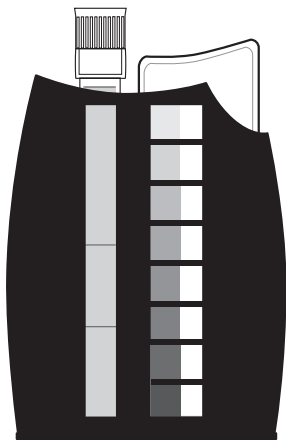
CODE 3354-01

QUANTITY	CONTENTS	CODE
50	*Nitrate #1 Tablets	*2799A-H
50	*Nitrate #2 CTA Tablets	*NN-3703A-H
2	Test Tubes, 2.5-10.0 mL, plastic, w/caps	0106
2	Protective Sleeves	0106-FP
1	Nitrate-Nitrogen Octa-Slide 2 Bar, 0-15 ppm	3494-01
1	Octa-Slide 2 Viewer	1101

*WARNING: Reagents marked with an * are considered to be potential health hazards. To view or print a Material Safety Data Sheet (MSDS) for these reagents go to www.lamotte.com. To obtain a printed copy, contact LaMotte by e-mail, phone or fax.

To order individual reagents or test kit components, use the specified code number










USE OF THE OCTA-SLIDE 2 VIEWER



The Octa-Slide 2 Viewer should be held so non-direct light enters through the back of the Viewer. Insert the reacted sample into the top of the Viewer. Slide the Octa-Slide 2 Bar into the Viewer and match the color of the reaction to the color standards.

WARNING! This set contains chemicals that may be harmful if misused. Read cautions on individual containers carefully. Not to be used by children except under adult supervision

PROCEDURE

<p>1.  Fill a test tube (0106) to the 5 mL line with sample water.</p>	<p>2.  Add one *Nitrate #1 Tablet (2799A).</p>	<p>3.  Cap and mix until tablet disintegrates.</p>
<p>4.  Add one *Nitrate #2 CTA Tablet (NN-3703A). Immediately slide the test tube into the Protective Sleeve (0106-FP).</p>	<p>5.  Cap and mix for two minutes to disintegrate the tablet.</p>	<p>6.  Wait 5 minutes. Remove the tube from the protective sleeve.**</p>
<p>7.  Insert Nitrate-Nitrogen Octa-Slide 2 Bar (3494-01) into the Octa-Slide 2 Viewer (1101)</p>	<p>8.  Insert test tube into Octa-Slide 2 Viewer (1101)</p>	<p>9.  Match sample color to a color standard. Record as ppm Nitrate Nitrogen.</p>
<p>NOTE: To convert to Nitrate, multiply results by 4.4. Record as ppm Nitrate. ** Nitrate #2 CTA Tablets (NN-3707) are sensitive to UV light. The Protective Sleeve (0106-FP) will protect the reaction from UV light. If testing indoors, there is no need to use the Protective Sleeve in this procedure.</p>		

LaMOTTE COMPANY

Helping People Solve Analytical Challenges®

PO Box 329 • Chestertown • Maryland • 21620 • USA
800-344-3100 • 410-778-3100 (Outside U.S.A.) • Fax 410-778-6394

Visit us on the web at www.lamotte.com